

Wear Property of Machined Ultra High Molecular Weight Polyethylene (UHMWPE) Acetabular Liner Product with CNC Milling

by Wahyu Dwi Lestari

Submission date: 17-Mar-2022 10:34AM (UTC+0700)

Submission ID: 1786088128

File name: JMEST_Wear_Property.pdf (521.14K)

Word count: 5837

Character count: 29643

Wear Property of Machined Ultra High Molecular Weight Polyethylene (UHMWPE) Acetabular Liner Product with CNC Milling

W D Lestari^{1*}, A T Danaryanto², A Nugroho³, R Ismail², J Jamari², A P Bayuseno²

¹Department of Mechanical Engineering, Faculty of Engineering, University of Pembangunan Nasional "Veteran" Jawa Timur,

Jl. Raya Rungkut Madya, Gunung Anyar, Surabaya, 60294, Indonesia

²Department of Mechanical Engineering, Faculty of Engineering, Diponegoro University,

Jl. Prof. Soedarto, Tembalang, Semarang, 50275, Indonesia

³PUTP (Pusat Unggulan Teknologi Plastik) Politeknik ATMI,

Jl. Mojo No.1, Karangasem, Laweyan, Surakarta, 57102, Indonesia

*Corresponding author: wahyu.dwi.tm@upnjatim.ac.id

ABSTRACT

UHMWPE has been used as a cushion in artificial hip joint for the last decades. The reliability of the components of a hip joint implant can be achieved by understanding their wear behavior. This study observed the tribological performance of the UHMWPE acetabular liner manufactured with a CNC milling machine on the femoral head made of SS 316L. Materials commonly used for tribo pairs in hip joint replacement. The wear tests were performed on a hip joint simulator in dry condition. The wear test is carried out by applying a constant load of 800N. Before and after the wear test, measurements of surface roughness and dimensional accuracy were carried out on the UHMWPE acetabular liner specimen. The relation between the surface roughness of the machining process and the wear rate is seen from the value of the wear depth and the wear coefficient obtained. The results showed that the machining process affects the surface roughness of the acetabular liner, where the roughness also affects the wear rate of acetabular liner product.

Copyright © 2021. Journal of Mechanical Engineering Science and Technology

Keywords: Acetabular liner, milling, surface roughness, UHMWPE, wear

15

I. Introduction

One of the vital parts of the human body is the hips [1]. The hip joint has an important role in the human body such as performing daily activities (walking, going downstairs, running, exercising, salat for muslim, etc.) because of its ability to transmit static and dynamic loads. Some of the problems that are often experienced by the hip joint include osteoarthritis, joint fractures, damage to the components of the femoral head and acetabular cup, and reduced synovial fluid in the joints. This makes the delivery painful, and an artificial hip implant is needed. The process of removing the diseased hip joint with an artificial hip joint that is similar in shape and function to the natural hip joint which is made of biocompatible materials, is known as Total Hip Replacement (THR). Many pairs of materials have been used for artificial hip joints. One of the most successful and widely used material pairs is UHMWPE against metal [2]. UHMWPE is the superior material used for today's artificial hip joint components [3]. As for metal components commonly used for biomedical applications is stainless steel 316 L due to its strength, thermal stability, high specific moduli and most importantly good wear resistance [4].



Despite its excellent properties, UHMWPE as a cushioning material in artificial joints has significant tribological problems. These problems include the appearance of wear debris of small size, which causes an adverse reaction in the surrounding tissue, resulting in aseptic loosening of the prosthesis components [5]. Because of this, UHMWPE materials have a limited lifespan of 15-20 years [6]. The wear behavior of hip implant materials depends on the condition of the surface, which can be obtained through the manufacturing process. Several scientific papers report on the effect of the manufacturing process on the characteristics of the resulting surface, which will certainly have an impact on the performance of the implant.

The application of multiple passes and cryogenic cooling to achieve high surface quality can improve wear performance [7], and also, there are correlations between surface integrity, surface topography, and material response [8]. Furthermore, the effect of surface roughness on the wear rate was also studied on the CoCrMo femoral head [9], MoM pairs material [10], and due to manufacturing process [11]. The wear of implant products is appreciated by the fact that the appearance of a large amount of wear has an adverse effect that can impact the life of the implant [12]. This wear rate can be reduced, and its life can be significantly extended by improving the quality of the bearing material [13-14]. Based on these reasons, research analysis and testing is an important part in the design and development of the hip joint to improve function and quality before the implantation process. Wear tests on hip prosthetics are usually performed on steady motion walking cycle obtained from the biomechanical literature [15-16]. The hip simulator is an experimentally proven tool for basic investigations and preclinical testing to minimize patient harm when receiving a new type of implant.


Hip joint simulator conducted to observe the changes in surface topography at the research stage of ball and socket friction pair [17], the wear performance of a non-cross linked UHMWPE pair versus two metal counterfaces, namely stainless steel (SS) and cobalt-chromium (CoCr) alloys, ceramic on ceramic [18], and cross linked ultra-high molecular weight polyethylene liners [19] on a variety of daily activities [16]. However, from some of the available literature, no one has paid attention to the influence of the UHMWPE acetabular liner machining process using a milling machine on the wear rate. Therefore, the purpose of this study was to observe the effect of the acetabular liner machining process for UHMWPE hip joints on wear behavior. The machining process is carried out using a CNC milling machine in dry conditions. Hip joint simulator was used to evaluate the wear rate of the UHMWPE acetabular liner from the machining process. Wear resistance tested for 30,000 cycles under walking cycle conditions. Wear quantity is calculated based on weight loss.

II. Material and Methods

A. Specimens Preparation

The hip joint consists of a ball and socket located between the acetabulum and the femur in the pelvis [20]. In this study, the acetabular liner component is derived from UHMWPE rod-shaped material which is manufactured using a CNC milling machine in dry conditions (Figure 1). The CNC milling machine used is YCM 1020 EV 20 with 3 axes. In this research, 9 samples of acetabular liner were produced with CNC milling machine cutting parameters such as feed rate, toolpath strategy, step over, and spindle speed [21]. The size of the UHMWPE acetabular liner formed is with an inner diameter of 28.2 mm. The result of this acetabular liner milling process must have a surface roughness below 2 μm and

dimensional tolerance in the range of +0.3 and -0.0 according to ASTM F2033-12. Furthermore, optimization was carried out on 9 samples of acetabular liner from the results of the manufacturing process to get 3 samples with the best roughness value. The 3 samples (Figure 2) of the acetabular liner from the optimization results were then tested for wear. Based on the measurement results, the size range of the acetabular liner specimen is obtained, namely the outer radius of 18.5 mm and the inner radius of 14.1 mm, where the three samples are still within the dimensional tolerance. The femoral head component is made of SS 316 L material with a diameter of 28 mm.

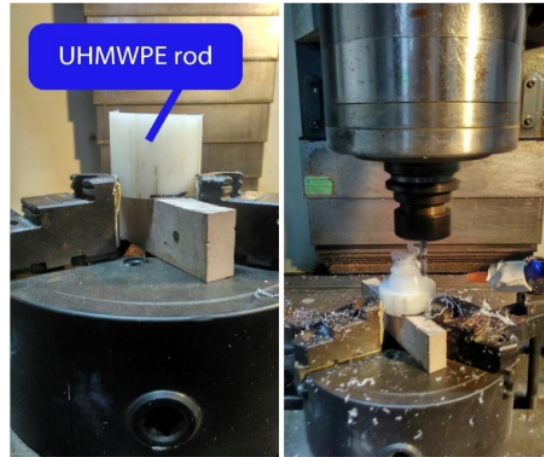

39 Fig. 1. Experimental set up for the milling of UHMWPE acetabular liner



Fig. 2. Acetabular liner

UHMWPE acetabular liner products resulting from the machining process are measured for surface roughness before wear testing is carried out. The process of measuring surface roughness was carried out using the Mark Surf PS1 surface roughness tester. The surface roughness measurement is carried out again after going through the wear test process, where the results can be seen in Table 1.

Table 1. The value of roughness of the inner acetabular liner before and after the test

Acetabular liner	Surface roughness	
	Before	After
Specimen 1	0.926	0.7756
Specimen 2	1.161	0.7182
Specimen 3	0.848	0.6786

The surface roughness values obtained from this study are in accordance with previous studies [22], which stated that the initial surface roughness of the polymer ranged from $0.4 \mu\text{m}$ - $2.2 \mu\text{m}$, but generally has a surface roughness level of about $1 \mu\text{m}$ - $2 \mu\text{m}$. In another study showed that the maximum initial surface roughness level of UHMWPE was $2 \mu\text{m}$ before the wear test was carried out [23-24].

B. Wear Test using Hip Joint Simulator

The prototype joint generated from the manufacturing process is then carried out preclinical testing using a simulator that is able to imitate motion behavior, biomechanics, and environmental conditions in the human body [24]. Tribological measurements in this study were carried out using a specially modified tribometer in the chamber to test the wear of the acetabular liner. The working principle of this tribometer machine is similar to the human hip joint, where there is a femoral head which is a parable of a human femur and a cup as a human pelvis. The maximum load that this testing machine can accept is 3000N. According to Hua et al. [25], the resultant force of the hip joint is 2500N, which is equivalent to 3-4 times the human body weight of 70 kg. The test design applied in this study is to provide as much insight as possible about the physical loading and motion that occurs between the femoral head and the acetabular liner upon contact.

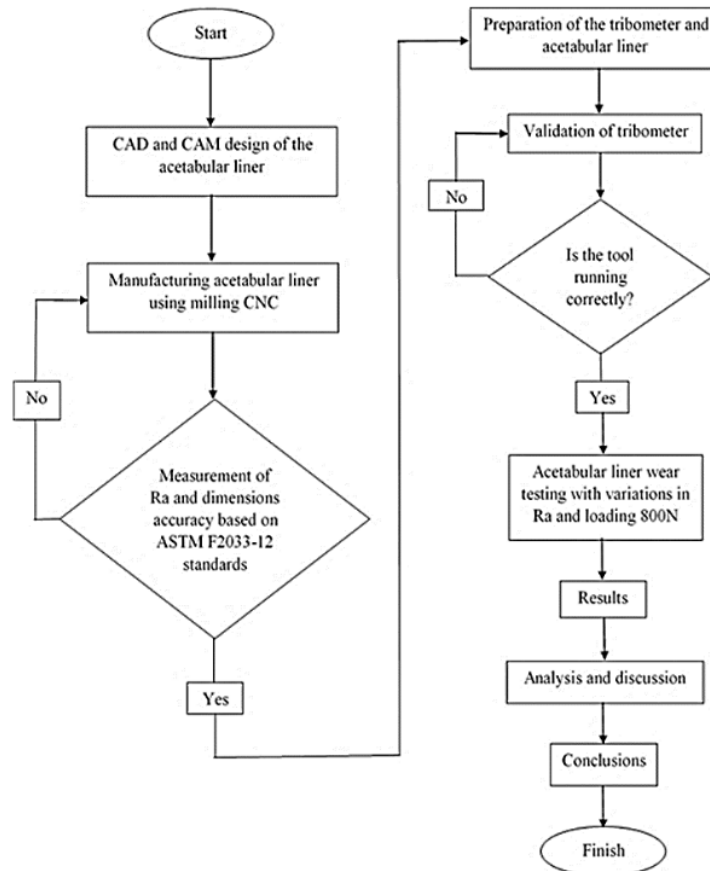


Fig. 3. Flowchart of the testing procedure of the UHMWPE acetabular liner using a tribometer

The testing parameters in this study are based on the ISO 14242 standard and previous research [26]. This study focuses on the effect of the UHMWPE acetabular liner machining process with CNC milling machine on the wear rate. The amount of force on the acetabular liner is determined by the weight of the human body. In this study, the amount of force applied is 800N which is based on the assumption of the patient's average weight [26]. The number of cycles applied in this test is 30000 cycles. The UHMWPE acetabular liner is attached to the SS 316L femoral head and encapsulated in the specimen chambers. The pair of specimens were sterilized first using 70% alcohol before being installed on the test machine. The wear testing process is carried out in dry conditions and at a temperature of 20⁰C. Gravimetric wear was obtained from the test results based on mass transformation. The entire experimental process in this study is shown in the flow chart in Figure 3.

C. Dimensional Accuracy Measurement

In addition to surface roughness, this study also measures the dimensional accuracy of the acetabular liner product. This measurement is carried out to ensure whether the resulting product conforms to the specified dimensional tolerance or not. Dimensional accuracy measurement using a coordinate measuring machine (CMM). Measurements are also carried out before and after the wear test process.

III. Results and Discussion

The results of this study will be used as a reference to improve the hip implant prototype. The resulting data in the form of the number of cycles and the depth of wear will be made into a graph of the relationship between the cycles and the depth of wear of the three test specimens. Changes in the volume of the acetabular liner were obtained by weighing. Changes in the initial and final weight data of the acetabular liner are shown in Table 2. Changes in the weight of the three samples prove that there is wear caused by the testing process in the walking cycle. Based on the weight change data contained in Table 2, it can be seen that test sample 2 has the largest weight change among the three samples. Furthermore, the data changes in the three samples are compared into a sine graph to determine the difference in the depth level of each specimen (Figure 4). The wear rate is determined by linear regression of the wear (mm) with the number of cycles. The wear depth (mm) of the UHMWPE acetabular liner is recorded as a function of the cycle length with a force of 800N.

Table 2. The initial and final weight of the acetabular liner

Specimens	Initial weight (g)	Final weight (g)	Weight change (g)
Specimen 1	6.8274	6.8260	0.0014
Specimen 2	6.3646	6.3350	0.0296
Specimen 3	6.1734	6.1720	0.0014

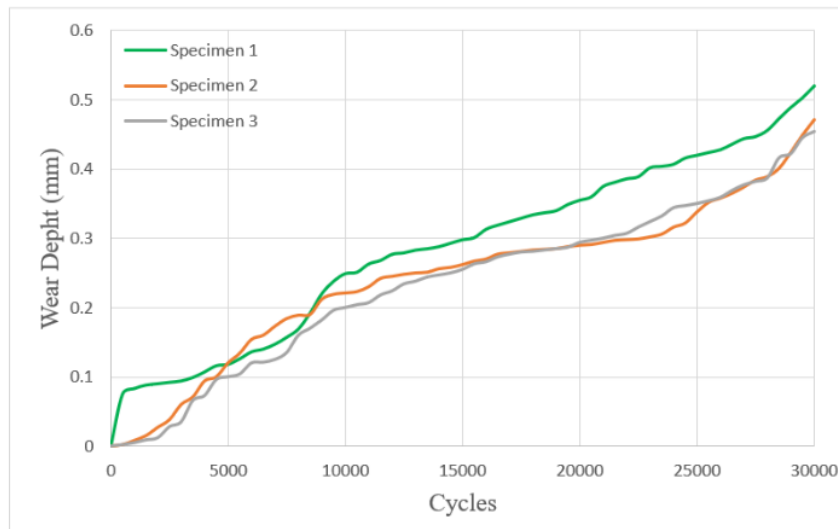


Fig. 4. Comparison of test results of 1,2,3 specimen with 800 N force

Based on Figure 5, it can be seen that the test results of the three specimens showed almost the same trend. The lowest wear depth is owned by specimen 3, where the largest wear depth is owned by specimen 1. There is a difference in the wear depth on the test results of specimen 1 from cycle 0 to cycle 3000 compared to specimen 2 and specimen 3. Furthermore, the trend of the three objects shows the same trend after cycle 3000 to cycle 30000. The test results in this study indicate that there are different wear values of each acetabular liner specimen, where this is influenced by the presence of different roughness as well. Based on the graph, the value of the depth of wear each specimen is obtained through 30000 cycles of wear testing. Each specimen has a wear depth of 0.52 mm, 0.471 mm, and 0.454 mm from specimen 1, specimen 2, and specimen 3, respectively.

An understanding of wear behavior is an urgent part of obtaining preclinical data on the prosthesis prior to implantation. In this regard, in this study, we conducted a wear test on a laboratory scale to determine the wear behavior of the acetabular liner from the machining process as a bearing on an artificial hip joint. Wear measurement is especially needed to measure new designs and materials because of the continuous need to manufacture new joints. One solution to get the right component prosthesis design is to take geometrical measurements before, during, and after wear testing. For this purpose, this study uses a coordinate measuring machine (CMM) to measure the dimensional accuracy of the acetabular liner specimen before and after the wear test. The results of dimensional accuracy measurements on the three acetabular liner specimens are presented in Table 3.

Table 3. The value of dimension accuracy of the inner acetabular liner before and after testing

Acetabular liner	Accuracy Dimensions	
	Before	After
Specimen 1	14.439 mm	14.331 mm
Specimen 2	14.470 mm	14.134 mm
Specimen 3	14.354 mm	14.228 mm

Uddin et al. [27], [14] their research, measured the wear of polyethylene acetabular liner with CMM where the average linear and volumetric wear rates were 0.13 mm/year and 37.18 mm³/year, respectively. Previous studies [28] also reported acetabular linear and volumetric wear rates with XLPE materials of 0.024 mm/year and 4.5 mm³/year, respectively. In this study, specimen 2 had the biggest difference between before and after the test, which was 0.336 mm during the testing of 30000 cycles. Furthermore, specimens 1 and specimens 3 had differences in accuracy dimensions of 0.108 mm and 0.126 mm, respectively. This result is bigger when compared to previous studies.

Validation is needed before carrying out the wear testing process using a tribometer machine to find out whether the tool used is valid enough to take data. The validation method [6] to calculate the wear coefficient value generated from the test using the Archad equation with the femoral head radius of 14 mm and the acetabular liner radius of 14.1 mm. The load used is equal to 800 N [17] th 30000 cycles. The value of the wear coefficient produced in this test is equal to $1.945 \times 10^{-4} \text{ mm}^3 \text{ N}^{-1} \text{ m}^{-1}$. This value is then compared with the results of research conducted by Dowson [29] by entering the research parameters in the formula. Dowson et al. [29] conducted a wear test and obtained two wear coefficient values, namely $1.35 \times 10^{-7} \text{ mm}^3 / \text{Nm}$ and $4.49 \times 10^{-7} \text{ mm}^3 \text{ N}^{-1} \text{ m}^{-1}$. The results of the validation can be seen in Figure 5 as for the wear depth formula [29], namely:

$$p = \frac{0.001186}{\pi} \left(\frac{kBN}{R_1} \right) \left[1 + \sqrt{1 + 1686\pi \frac{R_1(R_2 - R_1)}{kBN}} \right] \quad (1)$$

Where P is penetration or wear depth (mm), k is wear coefficient (mm³ N⁻¹ m⁻¹), B is Body weight (N), N is number of cycles (cycles), R₁ is femoral head radius (mm), and R₂ is acetabular liner radius (mm). The results show that there are differences in the test results where the wear value obtained is higher than that produced by Dowson when the cycle runs more than 4,500 cycles, but the trend is almost the same. Thus, it can be concluded that the tools used are valid enough to be used in conducting research.

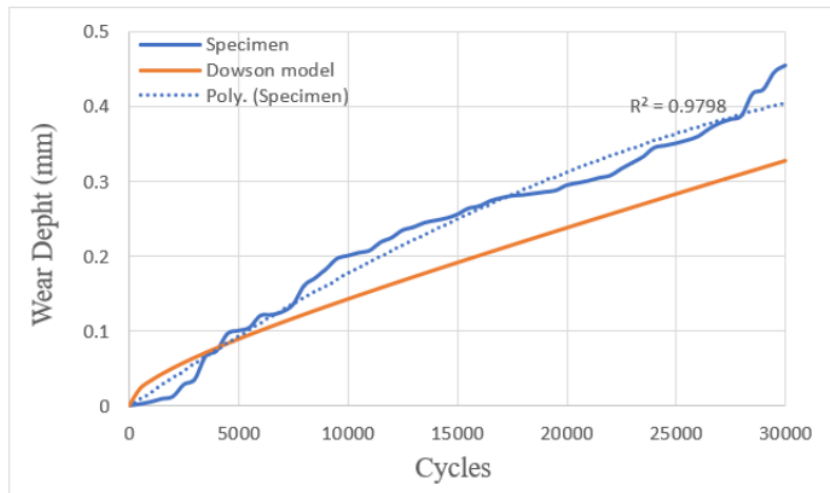


Fig. 5. Validation of test with Dowson model

The level of wear on biomedical components such as acetabular liners with variations in specifications and materials can be predicted through in vitro tests. The hip simulator test is the most commonly used tool by researchers to test the wear level of the acetabular liner with various parameter tests. In this study, the tribological behavior of the UHMWPE acetabular liner from the results of the CNC milling process with the femoral head pair was observed using a hip simulator based on the walking cycle. The difference in the wear rate of each specimen is caused by the difference in the surface roughness values obtained from the machining process [30]. This study took three samples of UHMWPE acetabular liner with the best roughness value based on the optimization results of nine samples made. The calculation results of the wear coefficient with the difference in the surface roughness values are shown in Figure 6, where the values of the wear volume and the level of penetration are presented in Table 4.

Table 4. Summary of UHMWPE wear behaviour in the simulator test condition.

Sample	Wear volume (mm ³)	Penetration rate (mm/year)	Wear coefficient (mm ³ N ⁻¹ m ⁻¹)
Specimen 1	102.98	0.33	2.78 x 10 ⁻⁴
Specimen 2	79.54	0.289	2.2 x 10 ⁻⁴
Specimen 3	75.46	0.279	1.95 x 10 ⁻⁴

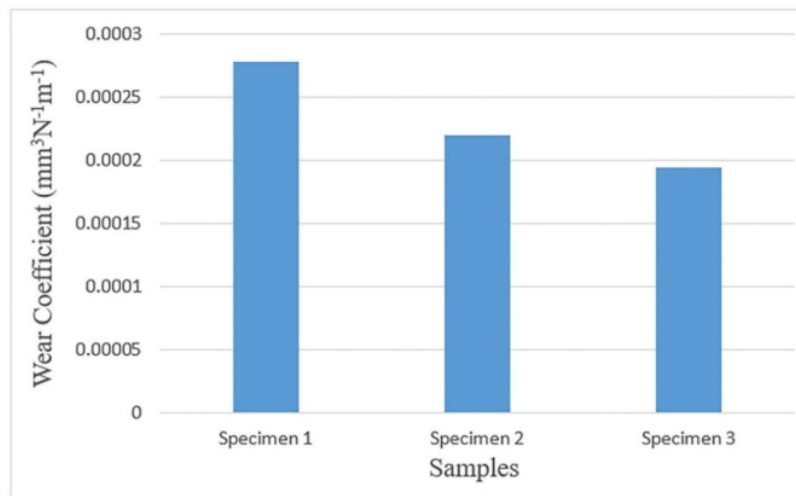


Fig. 6. Graph of wear coefficient calculations

Based on the graph in Figure 6, it can be seen that the highest wear coefficient value is found in specimen 1 of $2.78 \times 10^{-4} \text{ mm}^3 \text{ N}^{-1} \text{ m}^{-1}$. They were then followed by specimens 2 and 3 with values of $2.2 \times 10^{-4} \text{ mm}^3 \text{ N}^{-1} \text{ m}^{-1}$ and $1.95 \times 10^{-4} \text{ mm}^3 \text{ N}^{-1} \text{ m}^{-1}$, respectively. If observed, these results are related to the value of surface roughness. In accordance with previous studies [31], where the wear coefficient value produced is different in the contact test between UHMWPE which has an initial roughness value range of 1-2 μm with high-density alumina ceramic in dry conditions and lubricated with distilled water. After the wear test process, the surface roughness of the UHMWPE acetabular liner became smoother and

the value decreased from the initial surface roughness value (Table 2). This is as a result of the contact surface. This is also supported by previous research where the surface roughness value of UHMWPE was reduced from the initial value after going through a wear test process with a hip joint simulator for 5 million cycles [23-24]. Furthermore, the average surface roughness of UHMWPE acetabular liner decreased, ranging from 0.053 μm and 0.25 μm from the initial average surface roughness of 0.95 μm [32-33]. The observations results on the surface of the acetabular liner sample after testing 30,000 cycles indicate the presence of wear areas such as polish due to continuous loading. The surface of the acetabular liner may be scratched due to the appearance of a third body particle trapped between the polymer and metal surfaces. The scratch occurs because the counterface metallic is forced to move against the surface of the acetabular liner polymer and also a third body abrasion characterized by random directional scratches on the acetabular liner [23-24].

In this study, the wear mechanism that occurs is the third body abrasion with the test results in the form of wear depth and wear coefficient. The amount of wear in vivo generally ranges from 50-100 mg per year [33]. In various simulators, it is found that the wear value of polyethylene is in the range of 20-35 mg per 1 million cycles [34]. The total wear of the UHMWPE acetabular liner was 6378 mg for the acetabular liner with gamma irradiation and 7672 mg for the acetabular liner with EtO sterilization after going through five million cycles of testing [35-36]. With a linear wear rate of 0.16 mm/year, UHMWPE wear around 48 mg/106 cycles [23-24]. Furthermore, UHMWPE wear about 31.73 mg/million cycles and 15.20 mg/million cycles at 784 N and 392 N loadings, respectively [36]. An annual wear rate similar to the annual wear rate obtained from the observed popular MoP hip reconstruction, which was 25 mg per million cycles [37-38].

In this study, the lowest weight obtained after going through the wear testing process was 0.0014 g (1.4 mg/30000 cycles). The data obtained from this study cannot be compared directly with the results of wear experiments from the literature using a hip endoprosthesis simulator because the mechanism used is still simple on a laboratory scale [36]. The focus of this research is to examine the effect of the UHMWPE acetabular liner manufacturing process with CNC milling on surface roughness, where this roughness will affect the wear level of product for artificial hip joints. However, if plotted on a graph and calculated based on a linear equation of 1 million cycles, the wear rate of UHMWPE manufactured using a CNC milling machine is still in accordance with the in vivo wear rate provisions in the literature [38]. The wear tests performed in this study are in accordance with the literature, which describes the material wear of a commonly applied hip implant component under appropriate loading. Based on the test data and observations on the sample, it can be obtained that the surface roughness of the acetabular liner resulting from the milling process affects the depth and coefficient of wear.

IV. Conclusions

This study explores the influence of the UHMWPE acetabular liner manufacturing process with a CNC milling machine on the level of wear. Based on the results of the study, the conclusions obtained that the results of the wear coefficient calculation of the UHMWPE acetabular liner specimen indicate that the greater the surface roughness value of the acetabular liner, the greater the wear coefficient value, where the highest wear coefficient value is owned by specimen 1 of $2.57 \times 10^{-4} \text{ mm}^3/\text{Nm}$. The rate of wear depth and the wear coefficient of the UHMWPE acetabular liner produced in this study is influenced by the surface roughness value of the machining process with CNC milling.

Acknowledgment

The authors would like to acknowledge the LPPM of the University of Pembangunan Nasional Veteran Jawa Timur, which has supported financially for this publication. We also thank to the tribology laboratory of Diponegoro University and the PUTP ATMI for holding this experiment.

References

- [1] O. Hussain, S. S. Saleem, and B. Ahmad, "Friction and wear performance evaluation of UHMWPE using Taguchi based grey approach: A study on the influence of load and bio-serum lubrication," *Materials Chemistry and Physics*, vol. 239, no. April 2019, p. 121918, 2020, doi: 10.1016/j.matchemphys.2019.121918.
- [2] V. Saikko, V. Vuorinen, and H. Revitzer, "Analysis of UHMWPE wear particles produced in the simulation of hip and knee wear mechanisms with the RandomPOD system," *Biotribology*, vol. 1–2, pp. 30–34, 2015, doi: 10.1016/j.biotri.2015.03.002.
- [3] L. Hongtao, G. Shirong, C. Shoufan, and W. Shibo, "Comparison of wear debris generated from ultra high molecular weight polyethylene in vivo and in artificial joint simulator," *Wear*, vol. 271, no. 5–6, pp. 647–652, 2011, doi: 10.1016/j.wear.2010.11.012.
- [4] W. Qin, J. Kang, J. Li, W. Yue, Y. Liu, D. She, Q. Mao, and Y. Li, "Tribological behavior of the 316L stainless steel with heterogeneous lamella structure," *Materials*, vol. 11, no. 10, pp. 1–12, 2018, doi: 10.3390/ma11101839.
- [5] S. M. Kurtz, D. W. Macdonald, S. Kocagöz, M. Tohfafarosh, and D. Baykal, "Can Pin-on-Disk Testing Be Used to Assess the Wear Performance of Retrieved UHMWPE Components for Total Joint Arthroplasty?," *Biomed research international*, vol. 581812, pp. 1–6, 2014.
- [6] A. Laska, V. M. Archodoulaki, and B. Duscher, "Failure analysis of retrieved PE-UHMW acetabular liners," *Journal of the Mechanical Behavior of Biomedical Materials*, vol. 61, pp. 70–78, 2016, doi: 10.1016/j.jmbbm.2016.01.007.
- [7] S. Bruschi, R. Bertolini, A. Bordin, F. Medea, and A. Ghiotti, "Influence of the machining parameters and cooling strategies on the wear behavior of wrought and additive manufactured Ti6Al4V for biomedical applications," *Tribology International*, vol. 102, pp. 133–142, 2016, doi: 10.1016/j.triboint.2016.05.036.
- [8] D. Novovic, D. K. Aspinwall, R. C. Dewes, P. Bowen, and B. Griffiths, "The effect of surface and subsurface condition on the fatigue life of Ti – 25V – 15Cr – 2Al – 0.2C % wt alloy," *CIRP Annals - Manufacturing Technology*, vol. 65, no. 1, pp. 523–528, 2016, doi: 10.1016/j.cirp.2016.04.074.
- [9] S. Affatato, N. Freccero, and P. Taddei, "The biomaterials challenge : A comparison of polyethylene wear using a hip joint simulator," *Journal of the Mechanical Behavior of Biomedical Materials*, vol. 53, pp. 40–48, 2016, doi: 10.1016/j.jmbbm.2015.08.001.
- [10] R. K. Whittaker, H. S. Hothi, A. Eskelinen, G. W. Blunn, J. A. Skinner, and A. J. Hart, "Variation in Taper Surface Roughness for a Single Design Effects the Wear Rate in Total Hip Arthroplasty," *Journal Of Orthopaedic Research*, no. August, pp. 1784–1792, 2017, doi: 10.1002/jor.23456.

- [11] A. Turger, J. Köhler, B. Denkena, T. A. Correa, C. Becher, and C. Hurschler, "Manufacturing conditioned roughness and wear of biomedical oxide ceramics for all-ceramic knee implants," *BioMedical Engineering OnLine*, vol. 12, pp. 1–17, 2013.
- [12] D. J. Langton, T. J. Joyce, S. S. Jameson, J. Lord, M. V. Orsouw, J. P. Holland, A. V. F. Nargol, K. A. De Smet, "Adverse reaction to metal debris following hip resurfacing: The influence of component type, orientation and volumetric wear," *Journal of Bone and Joint Surgery - Series B*, vol. 93 B, no. 2, pp. 164–171, 2011, doi: 10.1302/0301-620X.93B2.25099.
- [13] C. Scemama, P. Anract, V. Dumaine, A. Babinet, J. P. Courpied, and M. Hamadouche, "Does vitamin E-blended polyethylene reduce wear in primary total hip arthroplasty: a blinded randomised clinical trial," *International Orthopaedics*, vol. 41, no. 6, pp. 1113–1118, 2017, doi: 10.1007/s00264-016-3320-2.
- [14] R. De Steiger, M. Lorimer, and S. E. Graves, "Cross-linked polyethylene for total hip arthroplasty markedly reduces revision surgery at 16 years," *Journal of Bone and Joint Surgery - American Volume*, vol. 100, no. 15, pp. 1281–1288, 2018, doi: 10.2106/JBJS.17.01221.
- [15] G. Valente, L. Pitto, R. Stagni, and F. Taddei, "Effect of lower-limb joint models on subject-specific musculoskeletal models and simulations of daily motor activities," *Journal of Biomechanics*, vol. 48, no. 16, pp. 4198–4205, 2015, doi: 10.1016/j.jbiomech.2015.09.042.
- [16] R. Viitala and V. Saikko, "Effect of random variation of input and various daily activities on wear in a hip joint simulator," *Journal of Biomechanics*, vol. 106, p. 109831, 2020, doi: 10.1016/j.jbiomech.2020.109831.
- [17] M. Niemczewska-wójcik, "Wear mechanisms and surface topography of artificial hip joint components at the subsequent stages of tribological tests," vol. 107, pp. 89–98, 2017, doi: 10.1016/j.measurement.2017.04.045.
- [18] M. de Fine, S. Terrando, M. Hintner, A. A. Porporati, and G. Pignatti, "Pushing Ceramic-on-Ceramic in the most extreme wear conditions: A hip simulator study," *Orthopaedics and Traumatology: Surgery and Research*, vol. 107, no. 1, 2021, doi: 10.1016/j.otsr.2020.05.003.
- [19] V. Saikko, "Effect of inward-outward rotation on hip wear simulation," *Journal of Biomechanics*, vol. 101, p. 109638, 2020, doi: 10.1016/j.jbiomech.2020.109638.
- [20] V. Jangid, A. K. Singh, and A. Mishra, "Wear simulation of artificial hip joints: Effect of materials," *Materials Today: Proceedings*, vol. 18, pp. 3867–3875, 2019, doi: 10.1016/j.matpr.2019.07.326.
- [21] W. D. Lestari, D. K. Nababan, R. Ismail, J. Jamari, and A. P. Bayuseno, "Dimensional Accuracy and Surface Roughness of Acetabular Liner with UHMWPE: Assessment Results between Compression Molding and CNC Milling," *International Review of Mechanical Engineering (I.R.E.M.E.)*, vol. 12, no. June, pp. 516–521, 2018.
- [22] D. Dowson and R. T. Harding, "The Wear Characteristics Of Ultrahigh Molecular Weight Polyethylene Against A High Density Alumina Ceramic Under Wet (Distilled Water) And Dry Conditions," *Wear*, vol. 75, pp. 313–331, 1982.

- [23] R. M. Trommer, M. M. Maru, W. L. O. Filho, V. P. S. Nykanen, C. P. Gouvea, B. S. Archanjo, E. H. M. Ferreira, R. F. Silva, C. A. Achete, "Multi-Scale Evaluation of Wear in UHMWPE-Metal Hip Implants Tested in a hip Joint Simulator," *Biotribology*, vol. 4, pp. 1–11, 2015, doi: 10.1016/j.biotri.2015.08.001.
- [24] L. Blunt, P. Bills, X. Jiang, C. Hardaker, and G. Chakrabarty, "The role of tribology and metrology in the latest development of bio-materials," *Wear*, vol. 266, no. 3–4, pp. 424–431, 2009, doi: 10.1016/j.wear.2008.04.015.
- [25] X. Hua, B. M. Wroblewski, Z. Jin, and L. Wang, "The effect of cup inclination and wear on the contact mechanics and cement fixation for ultra high molecular weight polyethylene total hip replacements," *Medical Engineering and Physics*, vol. 34, no. 3, pp. 318–325, 2012, doi: 10.1016/j.medengphy.2011.07.026.
- [26] A. L. L. Oliveira, R. G. Lima, E. G. Cueva, and R. D. Queiroz, "Comparative analysis of surface wear from total hip prostheses tested on a mechanical simulator according to standards ISO 14242-1 and ISO 14242-3," *Wear*, vol. 271, no. 9–10, pp. 2340–2345, 2011, doi: 10.1016/j.wear.2011.01.062.
- [27] M. S. Uddin, C. Y. E. Mak, and S. A. Callary, "Evaluating hip implant wear measurements by CMM technique," *Wear*, vol. 364–365, pp. 193–200, 2016, doi: 10.1016/j.wear.2016.07.017.
- [28] M. S. Uddin, "Wear Measurement and Assessment of Explanted Cross- Linked PE Acetabular Cups Using a CMM Wear Measurement and Assessment of Explanted Cross-Linked PE Acetabular Cups Using a CMM," *Tribology Transactions*, vol. 57 (5), no. July, pp. 37–41, 2014, doi: 10.1080/10402004.2014.911398.
- [29] D. Dowson and B. Jobbins, "An evaluation of the penetration polyethylene acetabular cups," *Wear*, vol. 164, pp. 162–164, 1993.
- [30] A. Essner, G. Schmidig, and A. Wang, "The clinical relevance of hip joint simulator testing : In vitro and in vivo comparisons," *Wear*, vol. 259, pp. 882–886, 2005, doi: 10.1016/j.wear.2005.02.105.
- [31] C. Liu, S. M. Green, N. D. Watkins, P. J. Gregg, and A. W. Mccaskie, "A preliminary hip joint simulator study of the migration of a cemented femoral stem," vol. 217, pp. 127–135, 2015.
- [32] X. Roussignol, C. Siedlecki, F. Duparc, F. Dujardin, and M. Ould-slimane, "Do temperature variations at the bearing surface during gait affect polyethylene wear in Chamley low-friction arthroplasty of the hip? Simulator study comparing UHMWPE and highly cross-linked polyethylene," *Orthopaedics & Traumatology: Surgery & Research*, vol. 102, no. 6, pp. 711–715, 2016, doi: 10.1016/j.otsr.2016.04.012.
- [33] V. Saikko, "Adverse condition testing with hip simulators," *Biotribology*, vol. 1–2, pp. 2–10, 2015, doi: 10.1016/j.biotri.2015.02.001.
- [34] M. P. Gispert, A. P. Serro, R. Colac, and B. Saramago, "Friction and wear mechanisms in hip prosthesis : Comparison of joint materials behaviour in several lubricants," *Wear*, vol. 260, pp. 149–158, 2006, doi: 10.1016/j.wear.2004.12.040.
- [35] S. Affatato, B. Bordini, C. Fagnano, P. Taddei, A. Tinti, and A. Toni, "Effects of the sterilisation method on the wear of UHMWPE acetabular cups tested in a hip joint simulator," vol. 23, pp. 1439–1446, 2002.

- [36] W. Shibo, G. Shirong, L. Hongtao, and X. Huang, "Wear behaviour and wear debris characterization of UHMWPE on alumina ceramic , stainless steel , CoCrMo and Ti6Al4V hip prostheses in a hip joint simulator," *Journal of Biomimetics, Biomaterials and Tissue Engineering*, vol. 7, pp. 7–25, 2010, doi: 10.4028/www.scientific.net/JBBTE.7.7.
- [37] C. R. Bragdon, D. O. Connor, J. D. Lowenstein, M. Jasty, and W. D. Syniuta, "The importance of multidirectional motion on the wear of polyethylene," *Proc Instn Mech Engrs*, vol. 210, 1996.
- [38] J. M. Kabo, J. S. Gebhard, G. Loren, H.C. Amstutz, "In vivo wear of polyethylene acetabular components," *The Journal of Bone and Joint Surgery*, vol. 75-B (2), pp. 254–258, 1993.

Wear Property of Machined Ultra High Molecular Weight Polyethylene (UHMWPE) Acetabular Liner Product with CNC Milling

ORIGINALITY REPORT

16%

SIMILARITY INDEX

1%

INTERNET SOURCES

15%

PUBLICATIONS

0%

STUDENT PAPERS

PRIMARY SOURCES

- 1** Ranjan, Prabhat, R. Balasubramaniam, and V.K. Suri. "Modelling and simulation of chemo-mechanical magnetorheological finishing (CMMRF) process", International Journal of Precision Technology, 2014. 2%
Publication

- 2** W. D. Lestari, D. K. Nababan, R. Ismail, J. Jamari, Athanasius P. Bayuseno. "Dimensional Accuracy and Surface Roughness of Acetabular Liner with UHMWPE: Assessment Results between Compression Molding and CNC Milling", International Review of Mechanical Engineering (IREME), 2018 1%
Publication

- 3** Dowson, D.. "The wear characteristics of ultrahigh molecular weight polyethylene against a high density alumina ceramic under wet (distilled water) and dry conditions", Wear, 19820115 1%
Publication

4

R.M. Trommer, M.M. Maru, W.L. Oliveira Filho, V.P.S. Nykanen et al. "Multi-Scale Evaluation of Wear in UHMWPE-Metal Hip Implants Tested in a hip Joint Simulator", *Biotribology*, 2015

Publication

1 %

5

Wang, Shi Bo, Shi Rong Ge, Hong Tao Liu, and Xiao Long Huang. "Wear Behaviour and Wear Debris Characterization of UHMWPE on Alumina Ceramic, Stainless Steel, CoCrMo and Ti6Al4V Hip Prostheses in a Hip Joint Simulator", *Journal of Biomimetics Biomaterials and Tissue Engineering*, 2010.

Publication

1 %

6

W D Lestari, R Ismail, J Jamari, A P Bayuseno. "Study on Wear Debris Characterization of Polycarbonate Urethane (PCU) as a Bearing of Artificial Hip Joint", *Journal of Physics: Conference Series*, 2021

Publication

<1 %

7

Wahyu Dwi Lestari, Luluk Edahwati, Wiliandi Saputro, Ahmad Khairul Faizin, Radissa Dzaky Issafira, Nurmala Shanti Dera. "Investigation The Effect of Clearance and Body Weight on The Contact Pressure of Metal on PCU Hip Prosthesis using Finite Element Method", *E3S Web of Conferences*, 2021

Publication

<1 %

8

Dowson, D.. "An evaluation of the penetration of ceramic femoral heads into polyethylene acetabular cups", *Wear*, 19930413

Publication

<1 %

9

Qingen Meng, Feng Liu, John Fisher, Zhongmin Jin. "Contact mechanics and lubrication analyses of ceramic-on-metal total hip replacements", *Tribology International*, 2013

Publication

<1 %

10

"UHMWPE Biomaterials for Joint Implants", Springer Science and Business Media LLC, 2019

Publication

<1 %

11

Advanced Tribology, 2010.

Publication

<1 %

12

Magdalena Niemczewska-Wójcik. "Wear mechanisms and surface topography of artificial hip joint components at the subsequent stages of tribological tests", *Measurement*, 2017

Publication

<1 %

13

Shawn Toh Ming Song, Ariyan Ashkanfar, Russell English, Glynn Rothwell. "Computational method for bearing surface wear prediction in total hip replacements",

<1 %

Journal of the Mechanical Behavior of Biomedical Materials, 2021

Publication

14

Bedard, Nicholas A., John J. Callaghan, Michael D. Stefl, Tyler J. Willman, Steve S. Liu, and Devon D. Goetz. "Fixation and Wear With a Contemporary Acetabular Component and Cross-Linked Polyethylene at Minimum 10-Year Follow-Up", *The Journal of Arthroplasty*, 2014.

Publication

<1 %

15

Rilo Berdin Taqriban, Ismoyo Haryanto, Dwi Basuki Wibowo, Rifky Ismail. "Hip Joint Implant Loading During Routine Activities of Elderly Indonesian", 2021 IEEE International Biomedical Instrumentation and Technology Conference (IBITeC), 2021

Publication

<1 %

16

Mohamad Raffi, N., and V. Srinivasan. "A study on wear behavior of γ -UHMWPE sliding against 316L stainless steel counter face", *Wear*, 2013.

Publication

<1 %

17

Isamu Sekiguchi, Kazuhisa Kubota, Yasushi Oyanagi, Masao Kosaka, Yoshihisa Sone. "Tribological properties of COPNA resin", *Wear*, 1992

Publication

<1 %

- | | | |
|----|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------|
| 18 | Sinnett-Jones, P.E.. "Micro-abrasion-corrosion of a CoCrMo alloy in simulated artificial hip joint environments", <i>Wear</i> , 200507/08
Publication | <1 % |
| 19 | Yoshimitsu Okazaki. "Selection of metals for biomedical devices", Elsevier BV, 2019
Publication | <1 % |
| 20 | eprints.soton.ac.uk
Internet Source | <1 % |
| 21 | journals.sagepub.com
Internet Source | <1 % |
| 22 | www.jbiomed.com
Internet Source | <1 % |
| 23 | E. Oral, S.M. Kurtz, O.K. Muratoglu. "Ultrahigh Molecular Weight Polyethylene Total Joint Implants*", Elsevier BV, 2011
Publication | <1 % |
| 24 | Fan, Xiaoqiang, and Liping Wang. "Highly Conductive Ionic Liquids toward High-Performance Space-Lubricating Greases", <i>ACS Applied Materials & Interfaces</i>
Publication | <1 % |
| 25 | Hasan Basri, A. Syahrom, A. T. Prakoso, D. Wicaksono, M. I. Amarullah, T. S. Ramadhoni, R. D. Nugraha. "The Analysis of Dimple Geometry on Artificial Hip Joint to the | <1 % |

Performance of Lubrication", Journal of Physics: Conference Series, 2019

Publication

26

M.S. Uddin, C.Y.E. Mak, S.A. Callary. "Evaluating hip implant wear measurements by CMM technique", Wear, 2016

Publication

<1 %

27

N. Shahemi, S. Liza, A.A Abbas, AM Merican. "LONG-TERM WEAR FAILURE ANALYSIS OF UHMWPE ACETABULAR CUP IN TOTAL HIP REPLACEMENT", Journal of the Mechanical Behavior of Biomedical Materials, 2018

Publication

<1 %

28

Raine Viitala, Vesa Saikko. "Effect of random variation of input and various daily activities on wear in a hip joint simulator", Journal of Biomechanics, 2020

Publication

<1 %

29

Saverio Affatato, Gianluca Bersaglia, Mirko Rocchi, Paola Taddei, Concezio Fagnano, Aldo Toni. "Wear behaviour of cross-linked polyethylene assessed in vitro under severe conditions", Biomaterials, 2005

Publication

<1 %

30

Uddin, M. S.. "Wear Measurement and Assessment of Explanted Cross-Linked PE Acetabular Cups using a CMM", Tribology Transactions, 2014.

<1 %

31

Volga Borah, Uddipta Bora, Utpal Jyoti Baishya, Boikuntha Pegu, Nitin Sahai. "Anatomization of wear behaviour of materials for total hip arthroplasty bearing surfaces: A review", Materials Today: Proceedings, 2021

Publication

<1 %

32

Affatato, S.. "Comparative study on the wear behaviour of different conventional and cross-linked polyethylenes for total hip replacement", Tribology International, 200808

Publication

<1 %

33

Fang Quan, Zhitong Chen, Huan Ye, Chuanhui Cui, Yunshuai Cui. "Study of the effect of surface roughness on fatigue strength of GH4169 based on indirect evaluation of the notch root radius", International Journal of Fatigue, 2021

Publication

<1 %

34

Leiming Gao, Zikai Hua, Robert Hewson. "Can a "pre-worn" bearing surface geometry reduce the wear of metal-on-metal hip replacements? – A numerical wear simulation study", Wear, 2018

Publication

<1 %

35

Lorenza Mattei, Francesca Di Puccio, Thomas J. Joyce, Enrico Ciulli. "Effect of size and

<1 %

dimensional tolerance of reverse total shoulder arthroplasty on wear: An in-silico study", Journal of the Mechanical Behavior of Biomedical Materials, 2016

Publication

36

Queiroz, R.D., A.L.L. Oliveira, F.C. Trigo, and J.A. Lopes. "A finite element method approach to compare the wear of acetabular cups in polyethylene according to their lateral tilt in relation to the coronal plane", Wear, 2013.

Publication

<1 %

37

Sawae, Yoshinori. "EFFECTS OF PHYSIOLOGICAL FACTORS ON WEAR OF UHMWPE FOR JOINT PROSTHESIS", Polymer Tribology, 2009.

Publication

<1 %

38

Shi Bo Wang, Shi Rong Ge, Hong Tao Liu, Xiao Long Huang. "Wear Behaviour and Wear Debris Characterization of UHMWPE on Alumina Ceramic, Stainless Steel, CoCrMo and Ti6Al4V Hip Prostheses in a Hip Joint Simulator", Journal of Biomimetics, Biomaterials and Tissue Engineering, 2010

Publication

<1 %

39

Stefania Bruschi, Rachele Bertolini, Fabrizio Medeossi, Andrea Ghiotti, Enrico Savio, Rajiv Shivpuri. "Case study: The application of machining-conditioning to improve the wear

<1 %

resistance of Ti6Al4V surfaces for human hip implants", Wear, 2018

Publication

40

Ulrike Mueller, Steffen Braun, Stefan Schroeder, Robert Sonntag, J. Philippe Kretzer. "Same Same but Different? 12/14 Stem and Head Tapers in Total Hip Arthroplasty", The Journal of Arthroplasty, 2017

Publication

<1 %

41

Vesa Saikko. "Adverse condition testing with hip simulators", Biotribology, 2015

Publication

<1 %

42

my.onexamination.com

Internet Source

<1 %

43

www.e3s-conferences.org

Internet Source

<1 %

44

"Advances in Mechanism and Machine Science", Springer Science and Business Media LLC, 2019

Publication

<1 %

45

Xian Wu, Mingyang Du, Jianyun Shen, Da Zeng, Bin Dai, Yuan Li, Hairong Wu. "Research on the Wear Performance of Artificial Knee Joint with Different Geometric Dimension", Journal of Medical and Biological Engineering, 2022

Publication

<1 %

Exclude quotes Off

Exclude matches Off

Exclude bibliography On